

CEMENT AND CONCRETE REFERENCE LABORATORY

PROFICIENCY SAMPLE PROGRAM

Final Report

C270 Masonry Mortar Proficiency Samples

Number 43 and Number 44



CCRL
Cement and Concrete
Reference Laboratory

October 2016

www.ccril.us



October 24, 2016

TO: Participants in the CCRL Masonry Mortar (ASTM C270) Proficiency Sample Program

SUBJECT: Final Report on Masonry Mortar Proficiency Samples No. 43 and No. 44

Enclosed is your copy of the final report on the test results for the pair of CCRL **Masonry Mortar Proficiency Samples** which were distributed in August 2016.

This report consists of a statistical Summary of Results, a set of general Scatter Diagrams, and associated detailed information. The Table of Results with test results and ratings for your laboratory can be downloaded at our website located at: <http://ccrl.us/>.

The CCRL Proficiency Sample Programs are intended for internal use by the laboratory as a tool to identify potential problems in laboratory procedures or test equipment and to initiate remedial actions. These programs are designed to complement the CCRL Laboratory Inspection Program as part of a total quality system. Care should be taken when using this program for any other purpose.

Additional samples of these two masonry mortars and other CCRL samples are available for purchase. These samples may be useful for equipment verification, technician training, and research. Contact CCRL for availability and price.

It is presently anticipated that the next Masonry Mortar Proficiency Samples will be distributed in August 2017.

Sincerely,

Robin K. Haupt
Supervisor, Proficiency Sample Program
Cement and Concrete Reference Laboratory

To: Participants in the CCRL C270 Masonry Mortar Proficiency Sample Program

FROM: Robin K. Haupt, Supervisor, PSP

SUBJECT: Explanation of Final Report on Results of Tests on C270 Masonry Mortar Proficiency Samples No. 43 and No. 44

This letter, and the material included with it, constitutes the final report and summary of results for the current pair of Masonry Mortar Proficiency Samples that were distributed in August 2016. This material includes a statistical Summary of Results, and a set of general Scatter Diagrams. If your laboratory was a participant in this program a Table of Laboratory Results (lab data and ratings) for your laboratory can be viewed and printed on the CCRL website.

An explanation of the program is contained in the paper: "Statistical Evaluation of Interlaboratory Cement Tests" by J. R. Crandall and R. L. Blaine [View Document](#), and "Statistical Aspects of the Cement Testing Program" by W.J. Youden [View Document](#), which can be found in Volume 59, Proceedings of the 62nd Annual Meeting of the Society, June 25, 1959, American Society for Testing and Materials.

Laboratory Ratings

Each laboratory receives an individualized Table of Results. The Table of Results shows the test title and the reporting unit in the first two columns. After that it lists the laboratory's results for the odd and even numbered samples, overall averages for the odd and even numbered samples, and the laboratory's ratings for the odd and even samples.

The ratings for the individual laboratory were determined in the manner described by Crandall and Blaine using a rating scale of 1 to 5 instead of 0 to 4. A rating of 0 is given for test results eliminated from calculations. The ratings have no valid standing beyond showing the difference between the individual laboratory result and the average for a particular test.

The following table details the relationship between the ratings and the averages.

Ratings	Range (Number of Standard Deviations)	Number (Per 100) of Laboratories achieving the rating ¹
5	Less than 1	69
4	1 to 1.5	18
3	1.5 to 2	9
2	2 to 2.5	3
1	Greater than 2.5	1

Note: The sign of the rating merely shows whether the result reported was greater or less than the average obtained.

¹Youden, W.J., "Statistical Aspects of the Cement Testing Program", Volume 59, *Proceedings of the 62nd Annual Meeting of the Society, June 25, 1959, American Society for Testing and Materials.*

Please note that individual laboratory ratings were not given for the flow of air content, compressive strength mortar, and initial water retention flow. Mortar flows in the range of 110 ± 5 are satisfactory, laboratories with flow values outside this range will be flagged as a "Labs Eliminated" on the scatter diagram. Averages, standard deviations, and a scatter diagram are provided for your information. This information may be a helpful indicator of a problem with flow table apparatus or mortar mixing procedures.

In cases where some laboratories' results are eliminated, averages, standard deviations, coefficients of variation, and the ratings of the other laboratories' results, are recalculated using the data remaining after the elimination. Since the laboratory ratings given are the results from this one series of tests, you need not attach too much significance to a single low rating, or pair of ratings, from this one series. A continuing tendency to get low ratings on several pairs of samples should lead a laboratory to consider the types of error, systematic and random, contribute to ratings that are low. Systematic error, which is indicated by low ratings with the same signs on each pair of samples, means a consistent error is occurring in equipment and/or test procedures. One indication of random error is low ratings on both samples with different signs. Since systematic error occurs with more regularity, its cause is generally easier to find than the cause of random error.

Summary of Results

Usually, averages, standard deviations, and coefficients of variation are given with all results reported, and then with one or more outlying results omitted. Sometimes, two or more recalculations with laboratories omitted, have been performed for the same test. In these cases, all of the laboratories omitted in previous recalculations are also omitted in subsequent ones. Results omitted are values that are more than three standard deviations from the mean of one or both samples. Often, elimination of these outlying results has little effect on the average, but may have a more pronounced effect on the standard deviation and coefficient of variation.

Scatter Diagrams

General scatter diagrams are supplied with this report. Crandall and Blaine describe the manner of preparing scatter diagrams, and their interpretation, in the paper published in the 1959 ASTM Proceedings.

Using the results received from each laboratory, a scatter diagram is generated for each test method by plotting the value for the odd numbered samples on the X, or horizontal axis, against the value for the even numbered samples on the Y, or vertical axis. To find your point, just plot as you would when plotting any scatter diagram. Vertical and horizontal dashed lines, which divide the diagrams into four sections or quadrants, place the average values for the odd and even numbered samples, respectively. The first line of print under the diagram includes the test number, as given on the data sheet, the test title, and the number of data points on the diagrams. The number of plotted points may not agree with the total number of data pairs included in the analysis because a few points may be off the diagram, and some points may represent several data pairs, which are identical. Laboratories whose points are off the diagram will have a rating of ± 1 or worst for that particular test.

As described in Crandall and Blaine, a tight circular pattern of points around the intersection of the median lines is the ideal situation. Stretching out of the pattern into the first (upper right) and third (lower left) quadrants, suggests some kind of bias, or tendency for laboratories to get high or low results on both samples. Examination of the scatter diagrams may indicate strong evidence of bias in many cases.

CCRL PROFICIENCY SAMPLE PROGRAM
Masonry Mortar Proficiency Samples No. 43 and No. 44

Final Report – October 24, 2016

SUMMARY OF RESULTS

Sample No.43

Sample No. 44

Test (unit)	#Labs	Average	S.D.	C.V.	Average	S.D.	C.V.
Air Content (percent)							
	35	16.0	2.3	15	18.6	3.2	17
	*33	16.4	1.2	7	19.1	1.9	10
* Labs Eliminated - 1589, 1993							
Air Content - Water (percent)							
	35	65.6	6.1	9.3	64.2	6.4	10.0
	*31	65.9	3.0	4.5	64.3	2.7	4.2
* Labs Eliminated - 575, 823, 828, 1993							
Air Content - Flow (percent)							
	35	109	5.7	5.2	109	4.9	4.5
	*34	110	2.9	2.6	110	2.1	1.9
* Labs Eliminated - 565							
Compressive Strength - 7 day (psi)							
	42	1064	668	63	901	510	57
	*38	868	248	29	765	269	35
* Labs Eliminated - 143, 1097, 1706, 3184							
Compressive Strength - 28 day (psi)							
	33	1450	969	67	1394	952	68
	*29	1124	229	20	1084	278	26
* Labs Eliminated - 143, 823, 1097, 1706							
Compressive Strength - Mix Water (percent)							
	39	65.6	6.1	9.3	64.5	6.6	10.2
	*36	66.1	3.7	5.6	64.9	4.0	6.2
* Labs Eliminated - 575, 828, 1993							
Compressive Strength - Flow (percent)							
	39	110	3.1	2.9	110	2.4	2.1
No Labs Eliminated for This Test							

CCRL PROFICIENCY SAMPLE PROGRAM
Masonry Mortar Proficiency Samples No. 43 and No. 44

Final Report – October 24, 2016


SUMMARY OF RESULTS

Sample No.43

Sample No. 44

Test (unit)	#Labs	Average	S.D.	C.V.	Average	S.D.	C.V.
Water Retention - Water (percent)							
	32	64.9	5.6	8.6	62.8	7.6	12.2
	*29	66.2	3.4	5.1	64.9	3.5	5.4
* Labs Eliminated - 565, 575, 828							
Water Retention - Initial Flow (percent)							
	32	111	2.8	2.5	110	2.2	2.0
No Labs Eliminated for This Test							
Water Retention - Final Flow (percent)							
	32	80	9.7	12.2	84	6.0	7.1
No Labs Eliminated for This Test							
Water Retention Value (percent)							
	32	72	8.8	12.2	77	5.0	6.5
No Labs Eliminated for This Test							

**CCRL Proficiency Sample Program
Air Content
MASONRY MORTAR Samples No. 43 and No. 44**

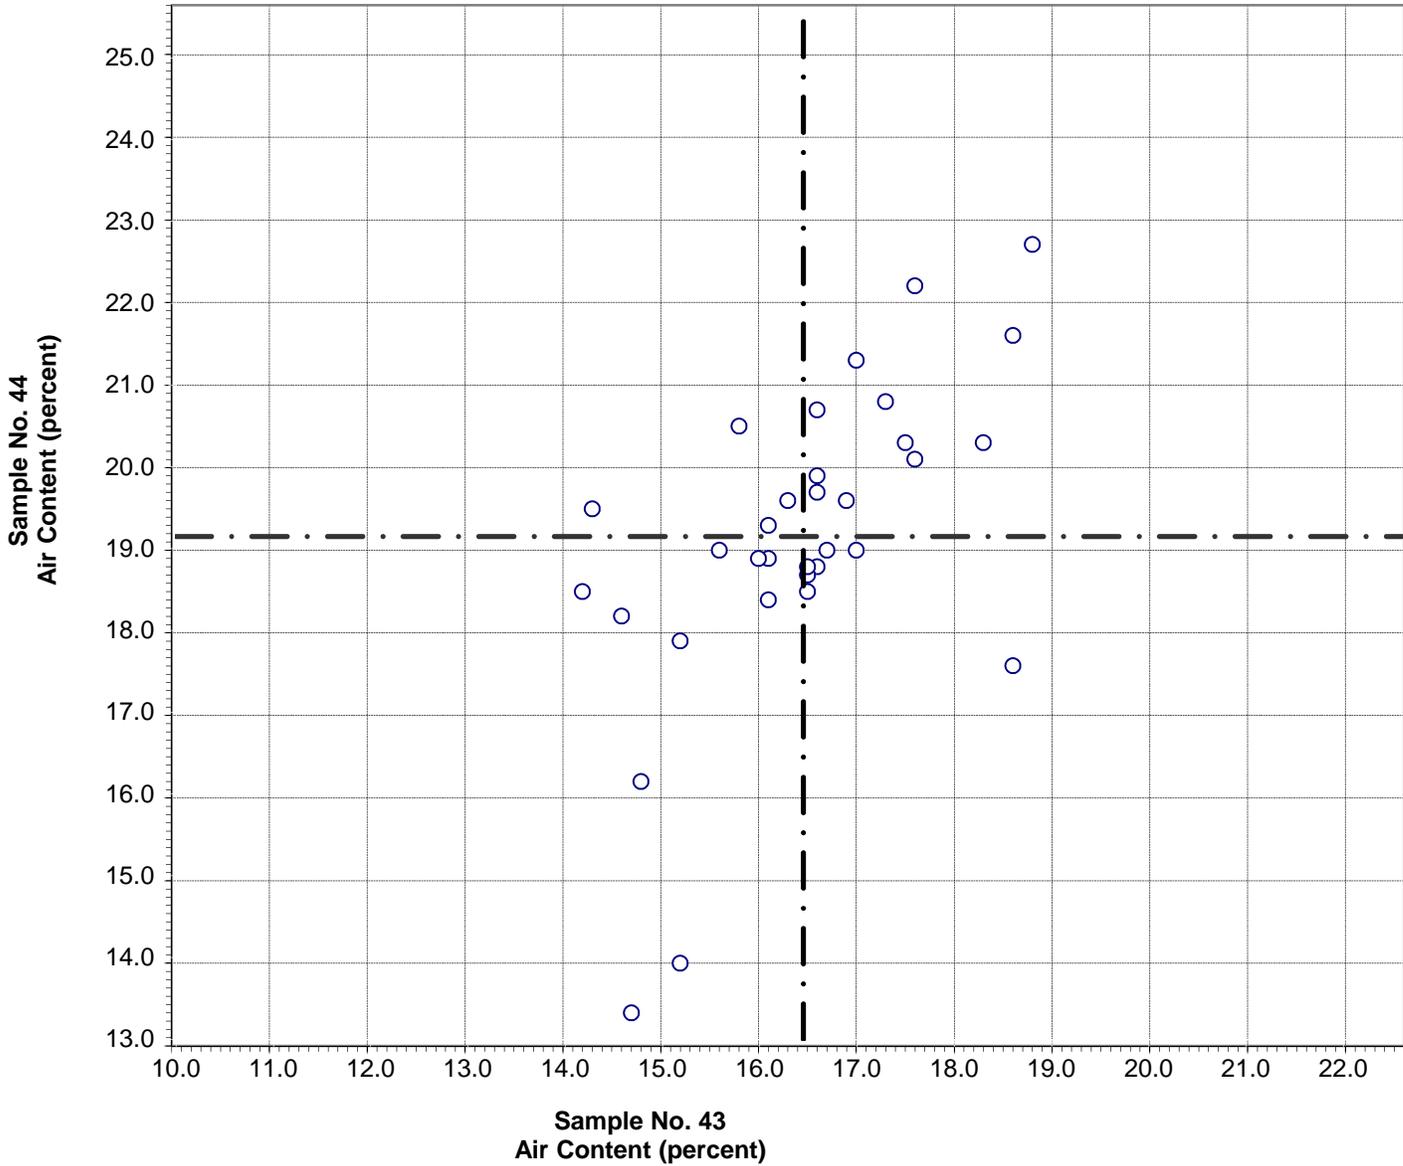


Test No. 170 Air Content 33 Points

Sample No. 43	Ave 16.4	S.D. 1.2	C.V. 7
Sample No. 44	Ave 19.1	S.D. 1.9	C.V. 10

Labs Eliminated: 1589, 1993

CCRL Proficiency Sample Program
Air Content - Water
MASONRY MORTAR Samples No. 43 and No. 44

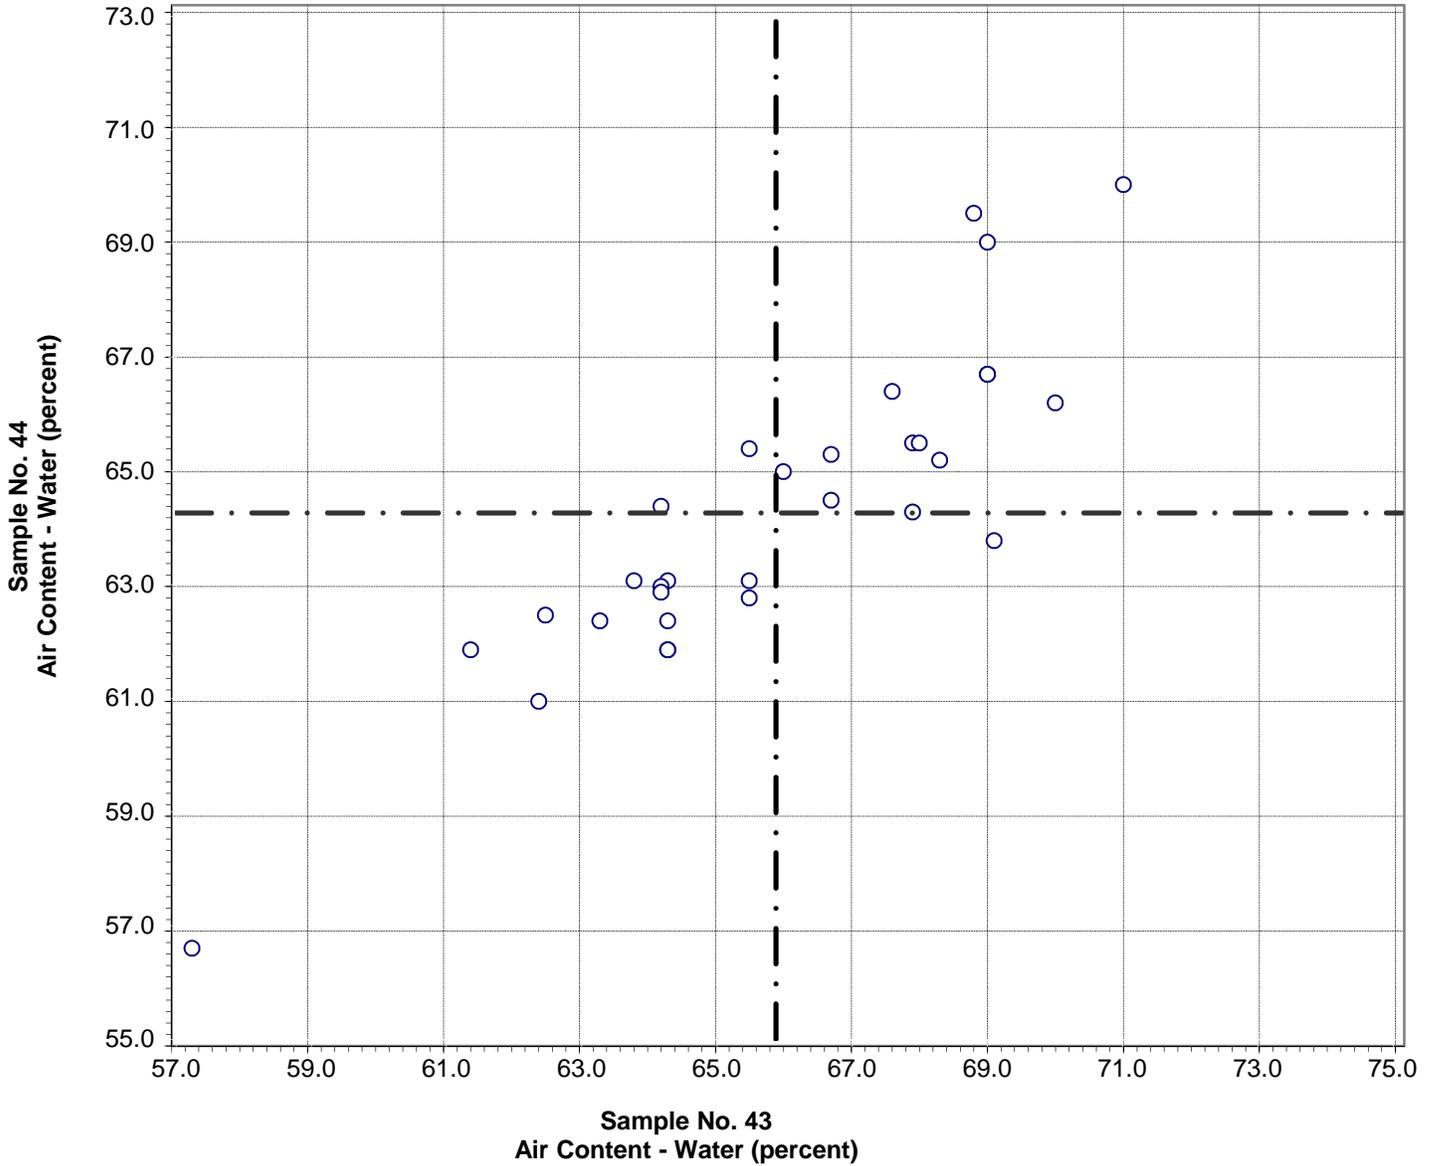


Test No. 180 Air Content - Water 31 Points

Sample No. 43	Ave 65.9	S.D. 3.0	C.V. 4.5
Sample No. 44	Ave 64.3	S.D. 2.7	C.V. 4.2

Labs Eliminated: 575, 823, 828, 1993

CCRL Proficiency Sample Program
Air Content - Flow
MASONRY MORTAR Samples No. 43 and No. 44

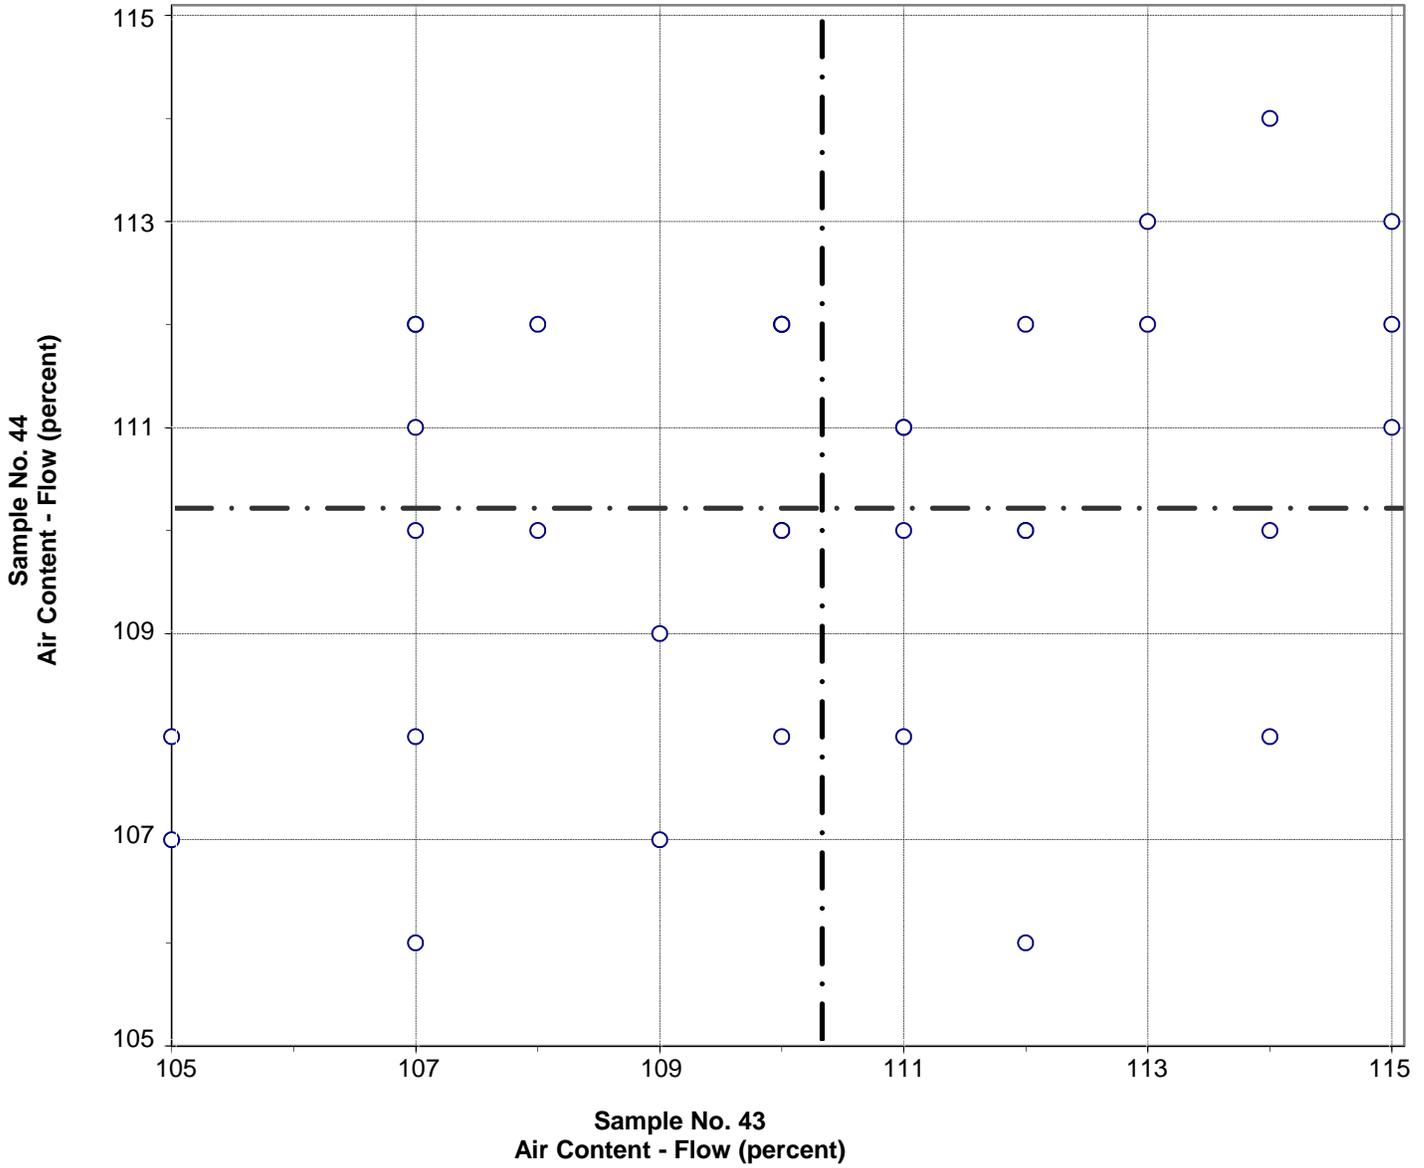


Test No. 190 Air Content - Flow 34 Points

Sample No. 43	Ave 110	S.D. 2.9	C.V. 2.6
Sample No. 44	Ave 110	S.D. 2.1	C.V. 1.9

Labs Eliminated: 565

**CCRL Proficiency Sample Program
Compressive Strength - 7 day
MASONRY MORTAR Samples No. 43 and No. 44**

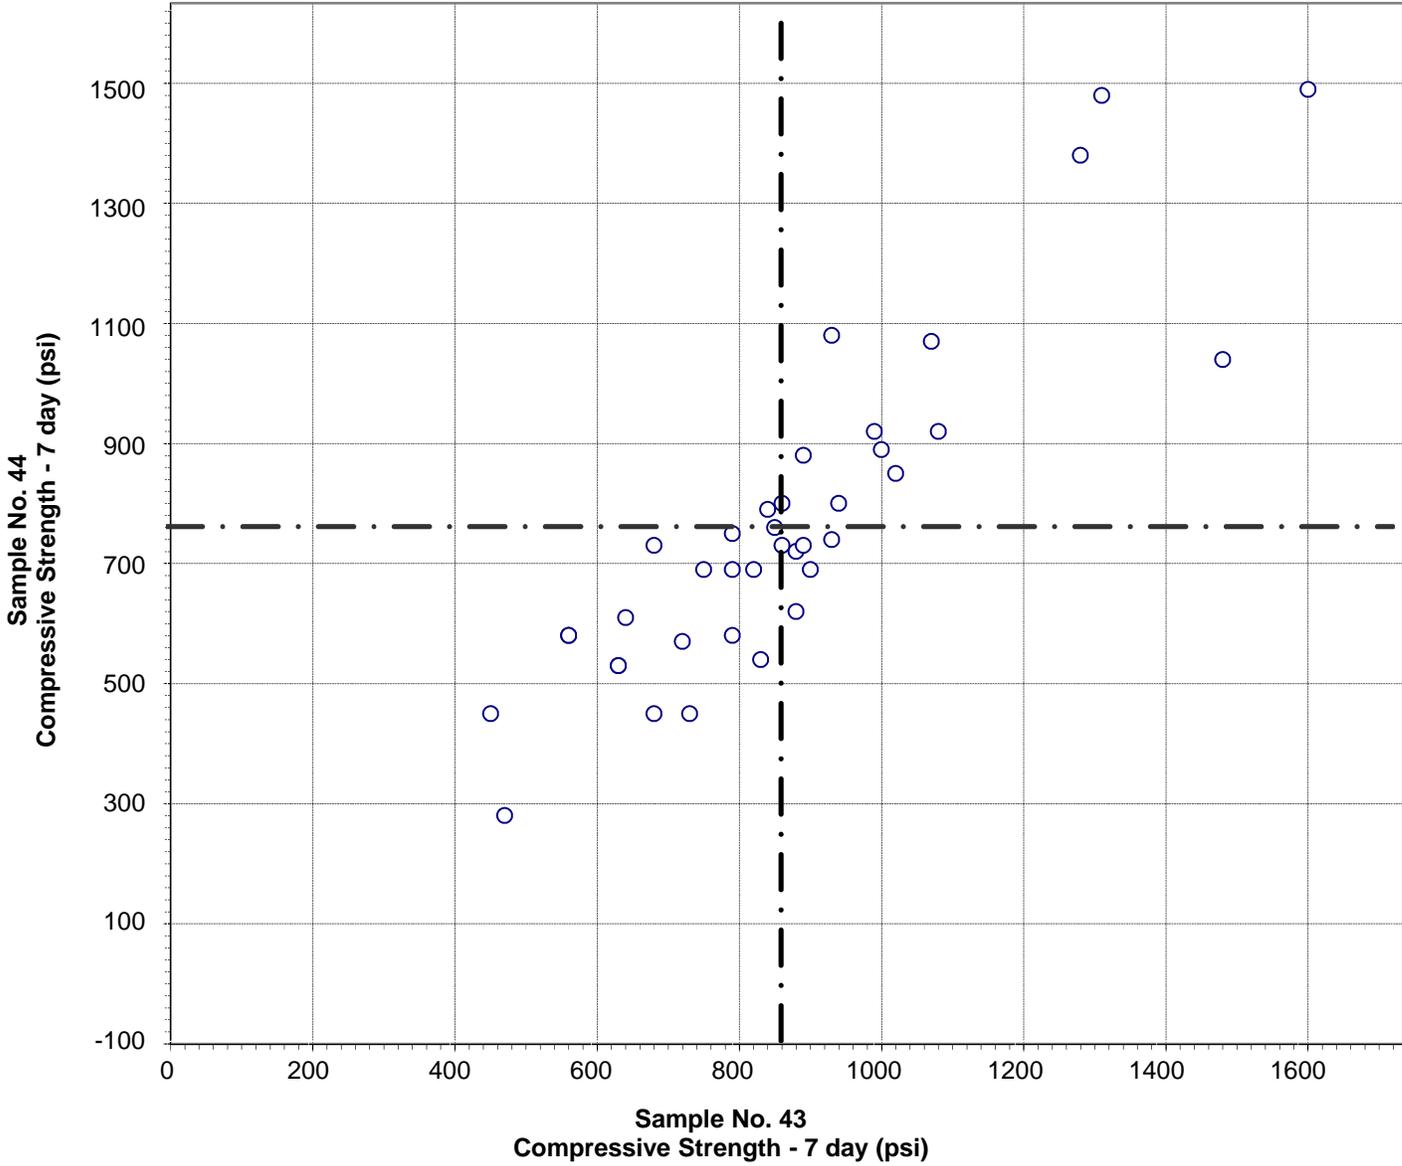


Test No. 210 Compressive Strength - 7 day 38 Points

Sample No. 43	Ave 868	S.D. 248	C.V. 29
Sample No. 44	Ave 765	S.D. 269	C.V. 35

Labs Eliminated: 143, 1097, 1706, 3184

**CCRL Proficiency Sample Program
Compressive Strength - 28 day
MASONRY MORTAR Samples No. 43 and No. 44**

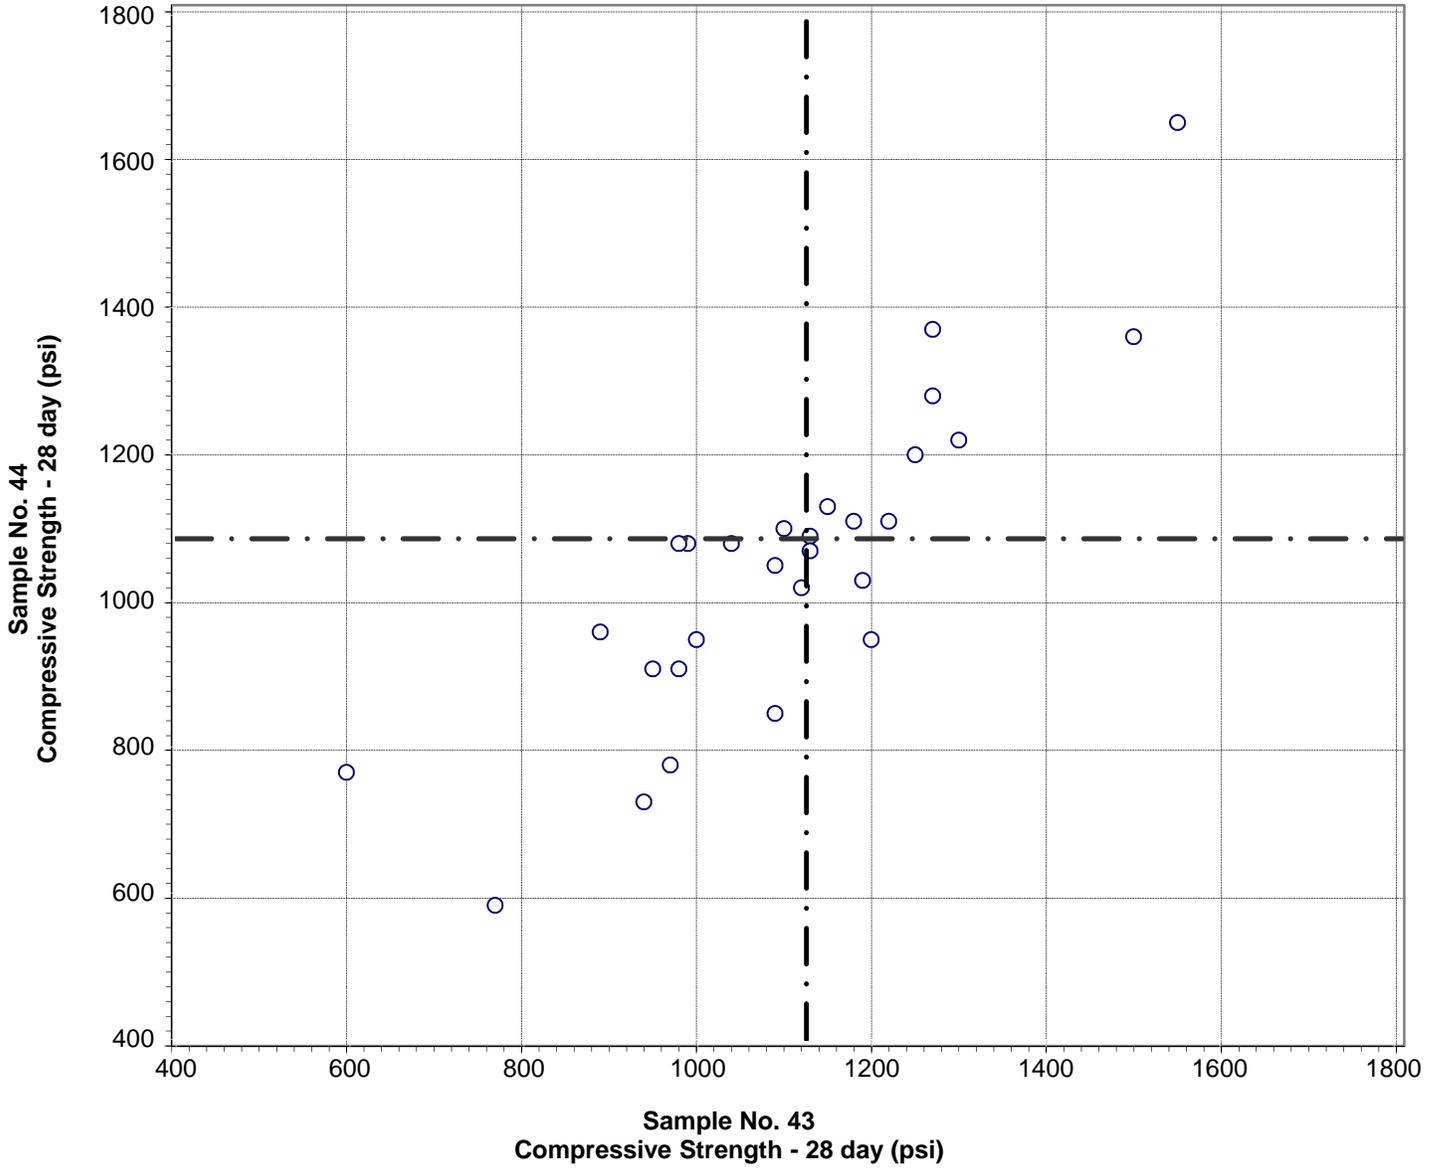


Test No. 211 Compressive Strength - 28 day 28 Points

Sample No. 43	Ave 1124	S.D. 229	C.V. 20
Sample No. 44	Ave 1084	S.D. 278	C.V. 26

Labs Eliminated: 143, 823, 1097, 1706

Labs off Diagram: 575

**CCRL Proficiency Sample Program
Compressive Strength - Mix Water
MASONRY MORTAR Samples No. 43 and No. 44**

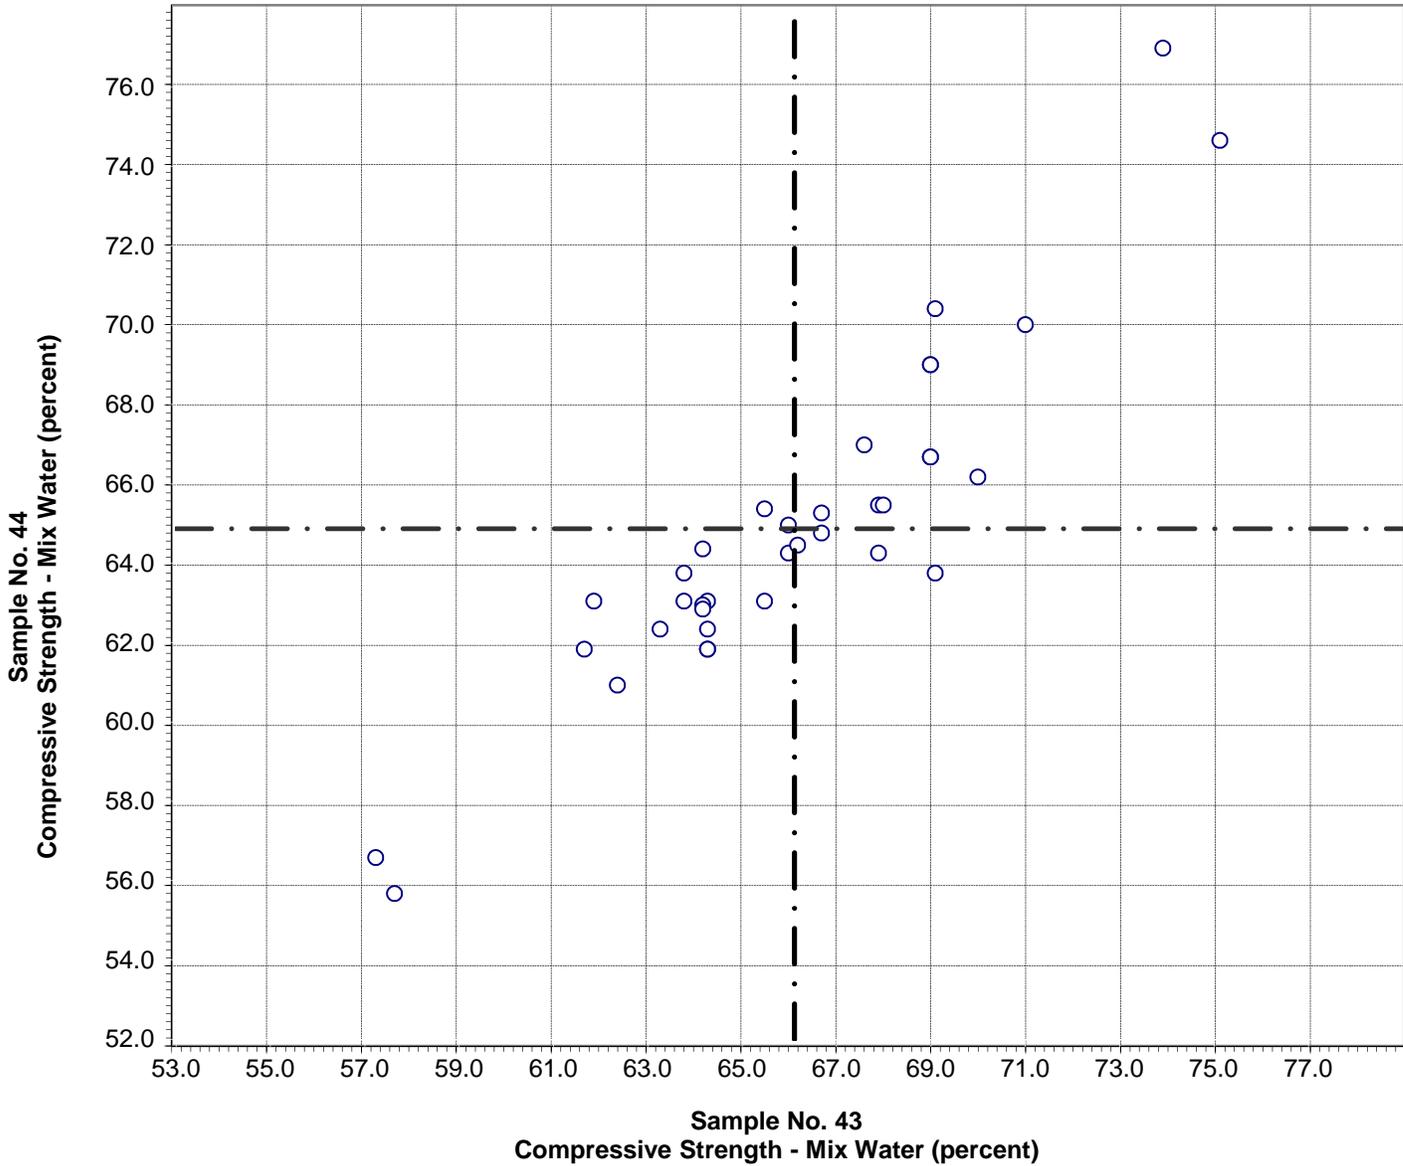


Test No. 220 Compressive Strength - Mix Water 36 Points

Sample No. 43	Ave 66.1	S.D. 3.7	C.V. 5.6
Sample No. 44	Ave 64.9	S.D. 4.0	C.V. 6.2

Labs Eliminated: 575, 828, 1993


**CCRL Proficiency Sample Program
Compressive Strength - Flow
MASONRY MORTAR Samples No. 43 and No. 44**

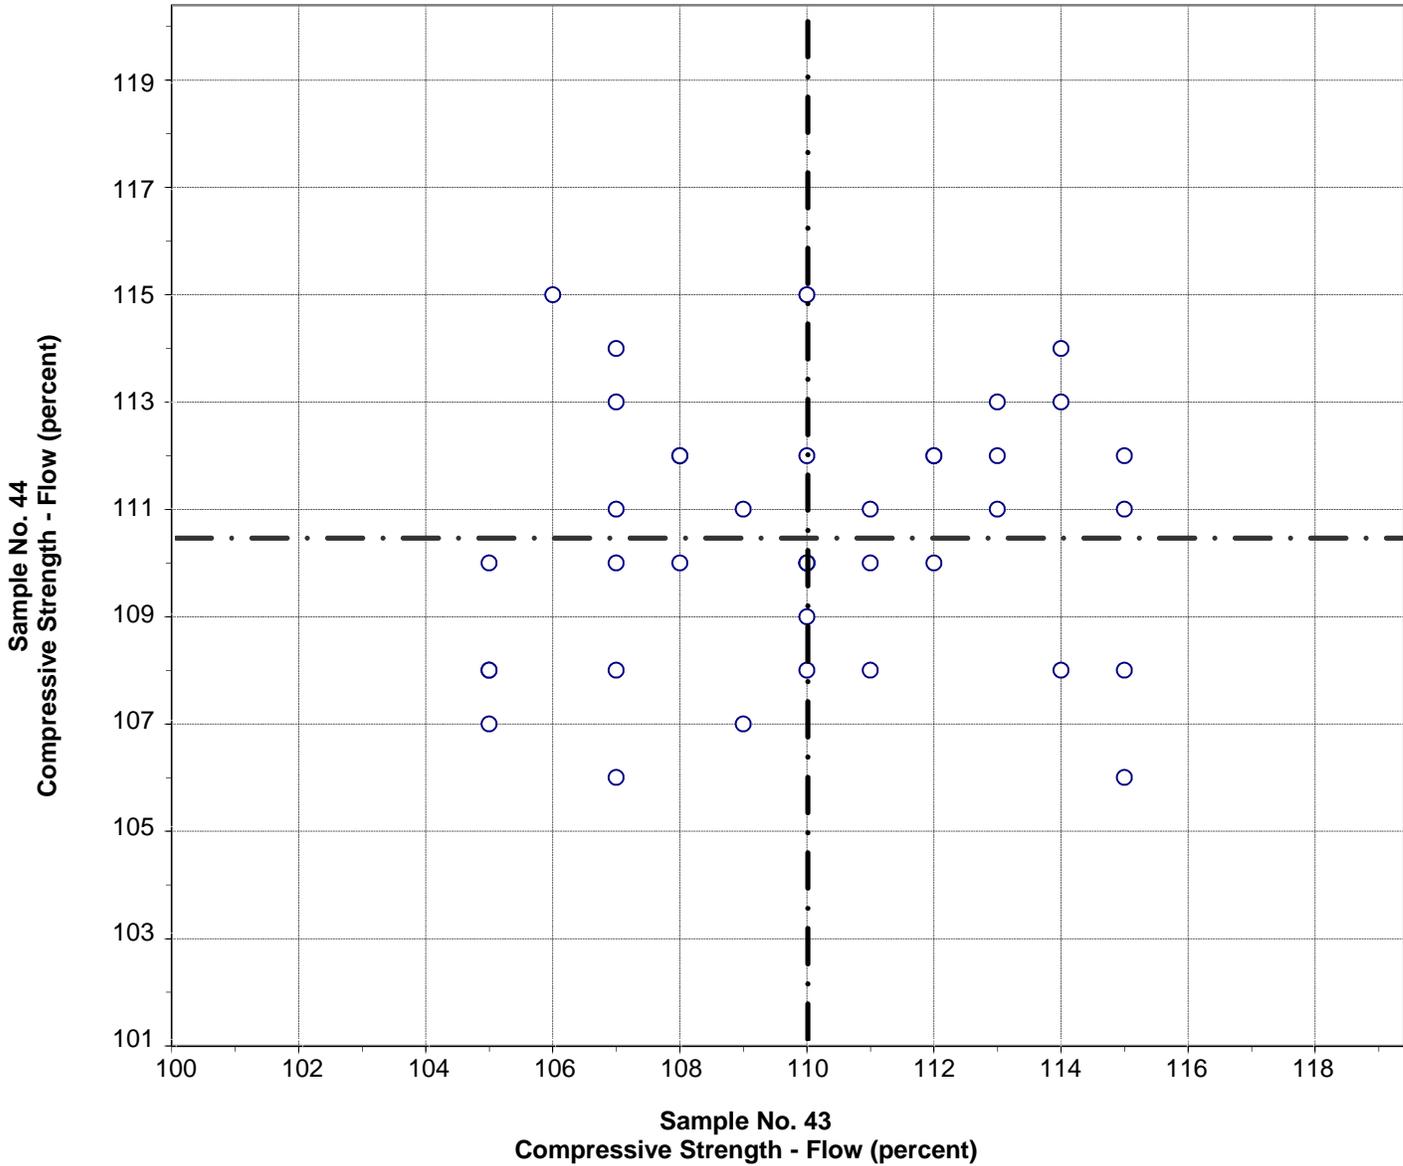

Test No. 230 Compressive Strength - Flow 39 Points

Sample No. 43	Ave 110	S.D. 3.1	C.V. 2.9
Sample No. 44	Ave 110	S.D. 2.4	C.V. 2.1

**CCRL Proficiency Sample Program
Water Retention - Water
MASONRY MORTAR Samples No. 43 and No. 44**

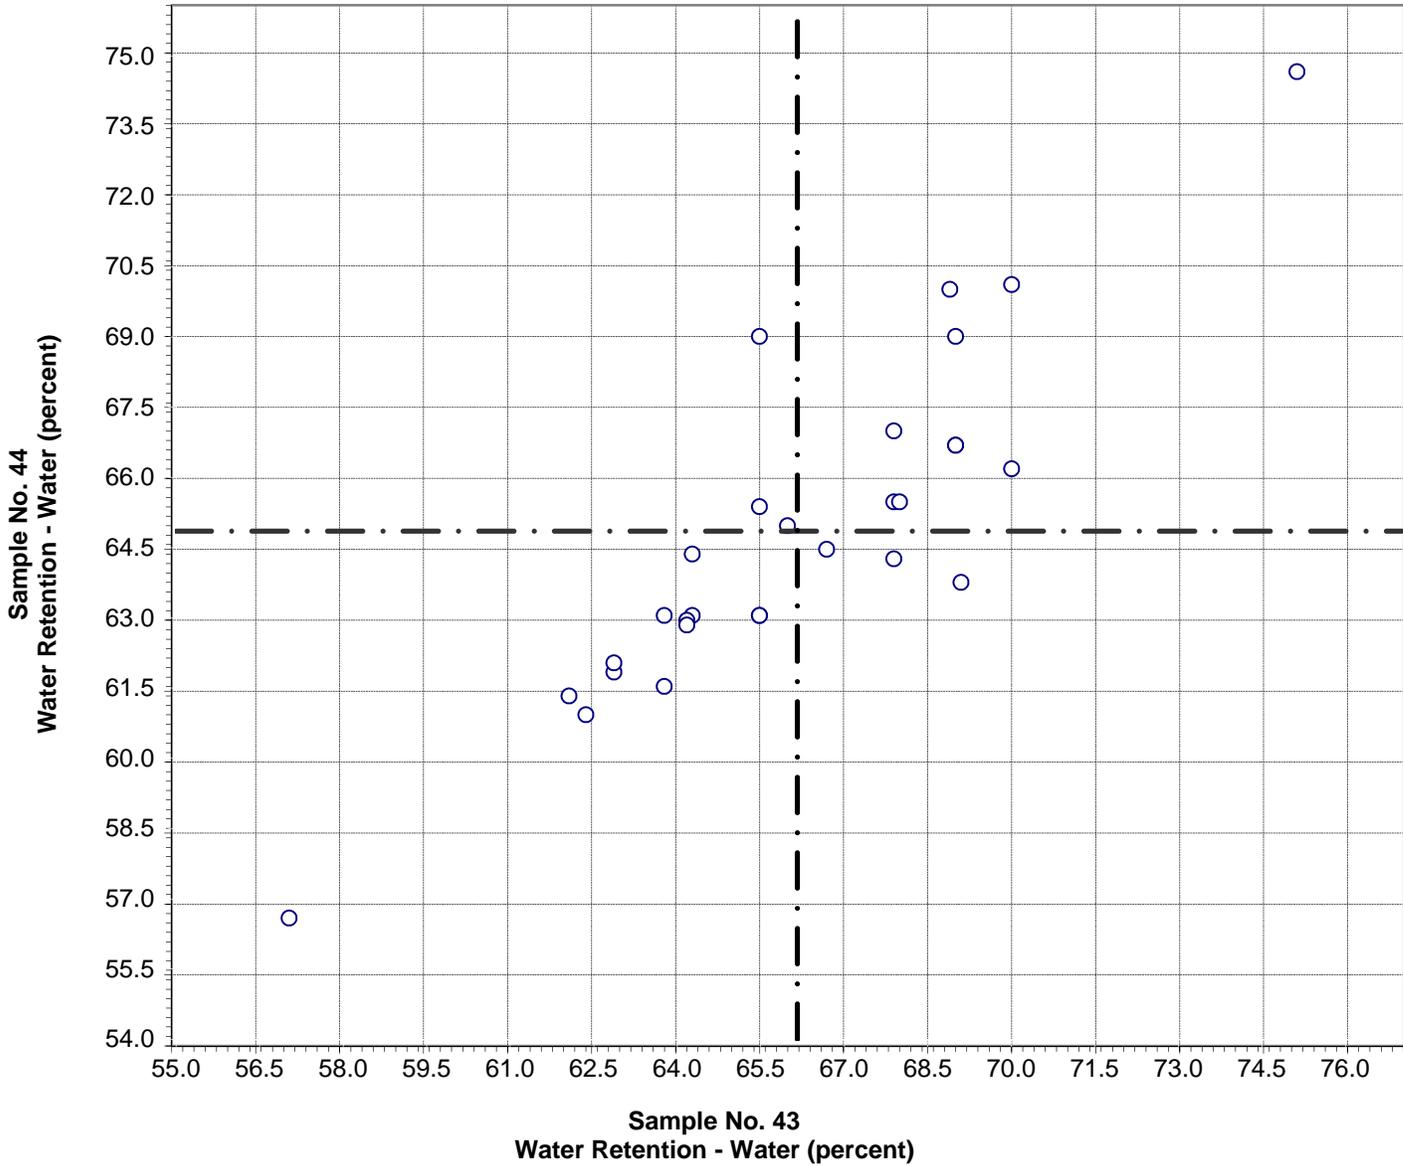


Test No. 330 Water Retention - Water 29 Points

Sample No. 43	Ave 66.2	S.D. 3.4	C.V. 5.1
Sample No. 44	Ave 64.9	S.D. 3.5	C.V. 5.4

Labs Eliminated: 565, 575, 828


**CCRL Proficiency Sample Program
Water Retention - Initial Flow
MASONRY MORTAR Samples No. 43 and No. 44**

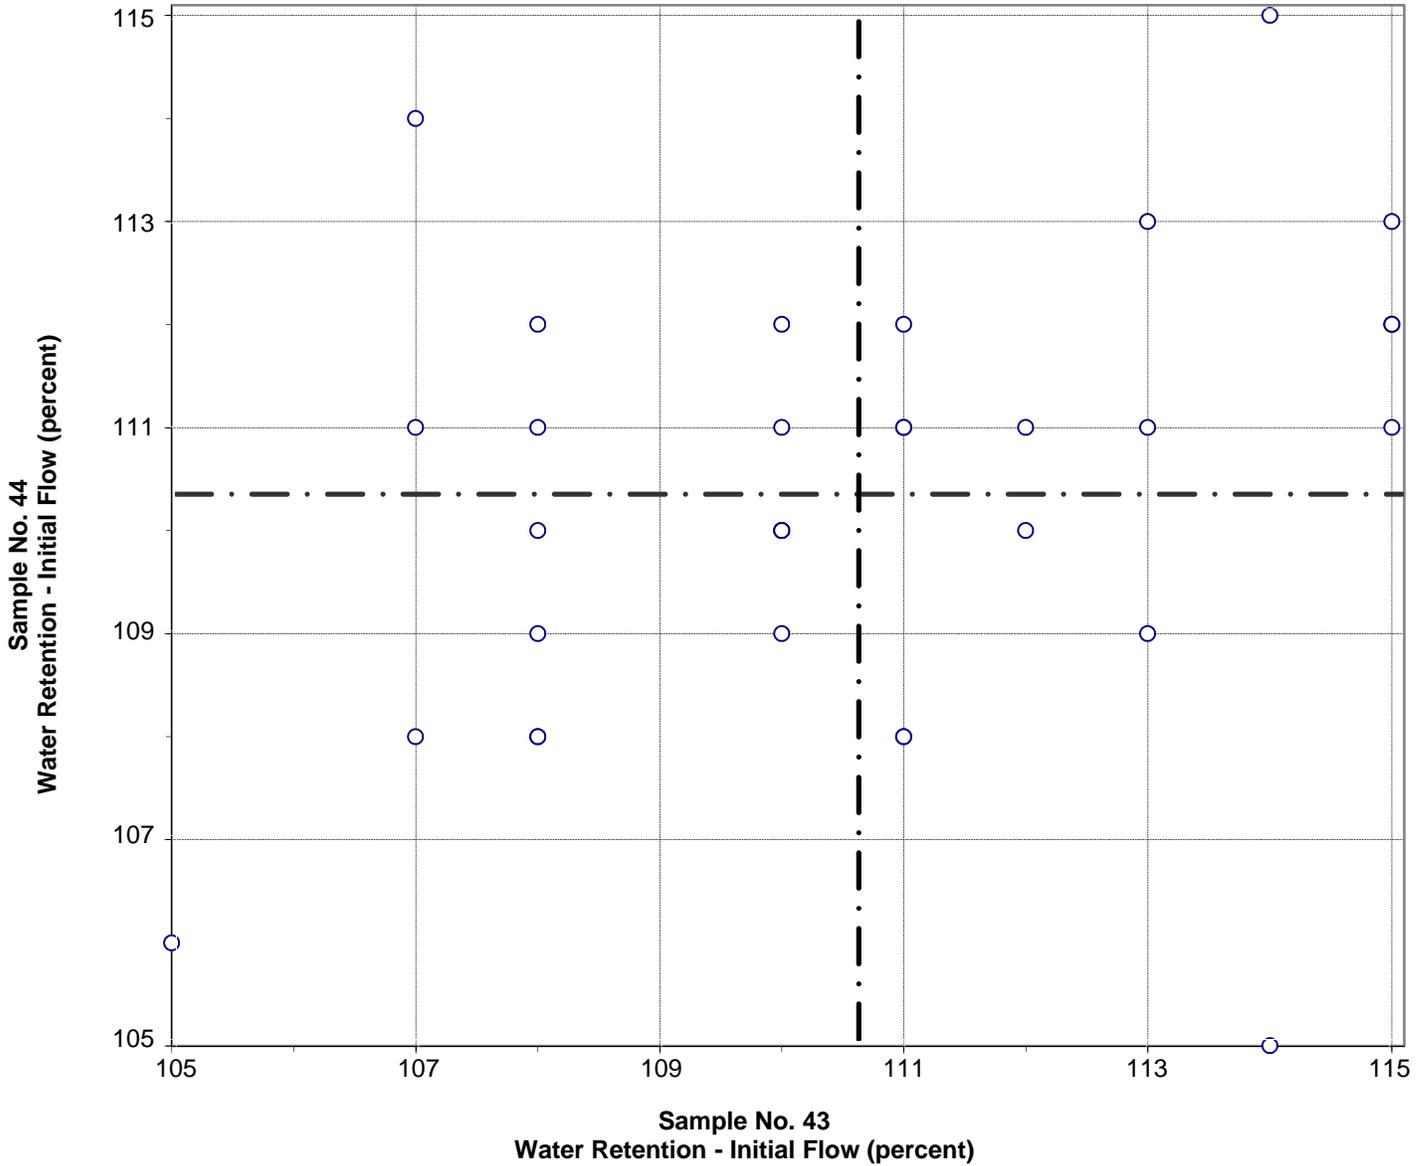

Test No. 331 Water Retention - Initial Flow 32 Points

Sample No. 43	Ave 111	S.D. 2.8	C.V. 2.5
Sample No. 44	Ave 110	S.D. 2.2	C.V. 2.0


**CCRL Proficiency Sample Program
Water Retention - Final Flow
MASONRY MORTAR Samples No. 43 and No. 44**

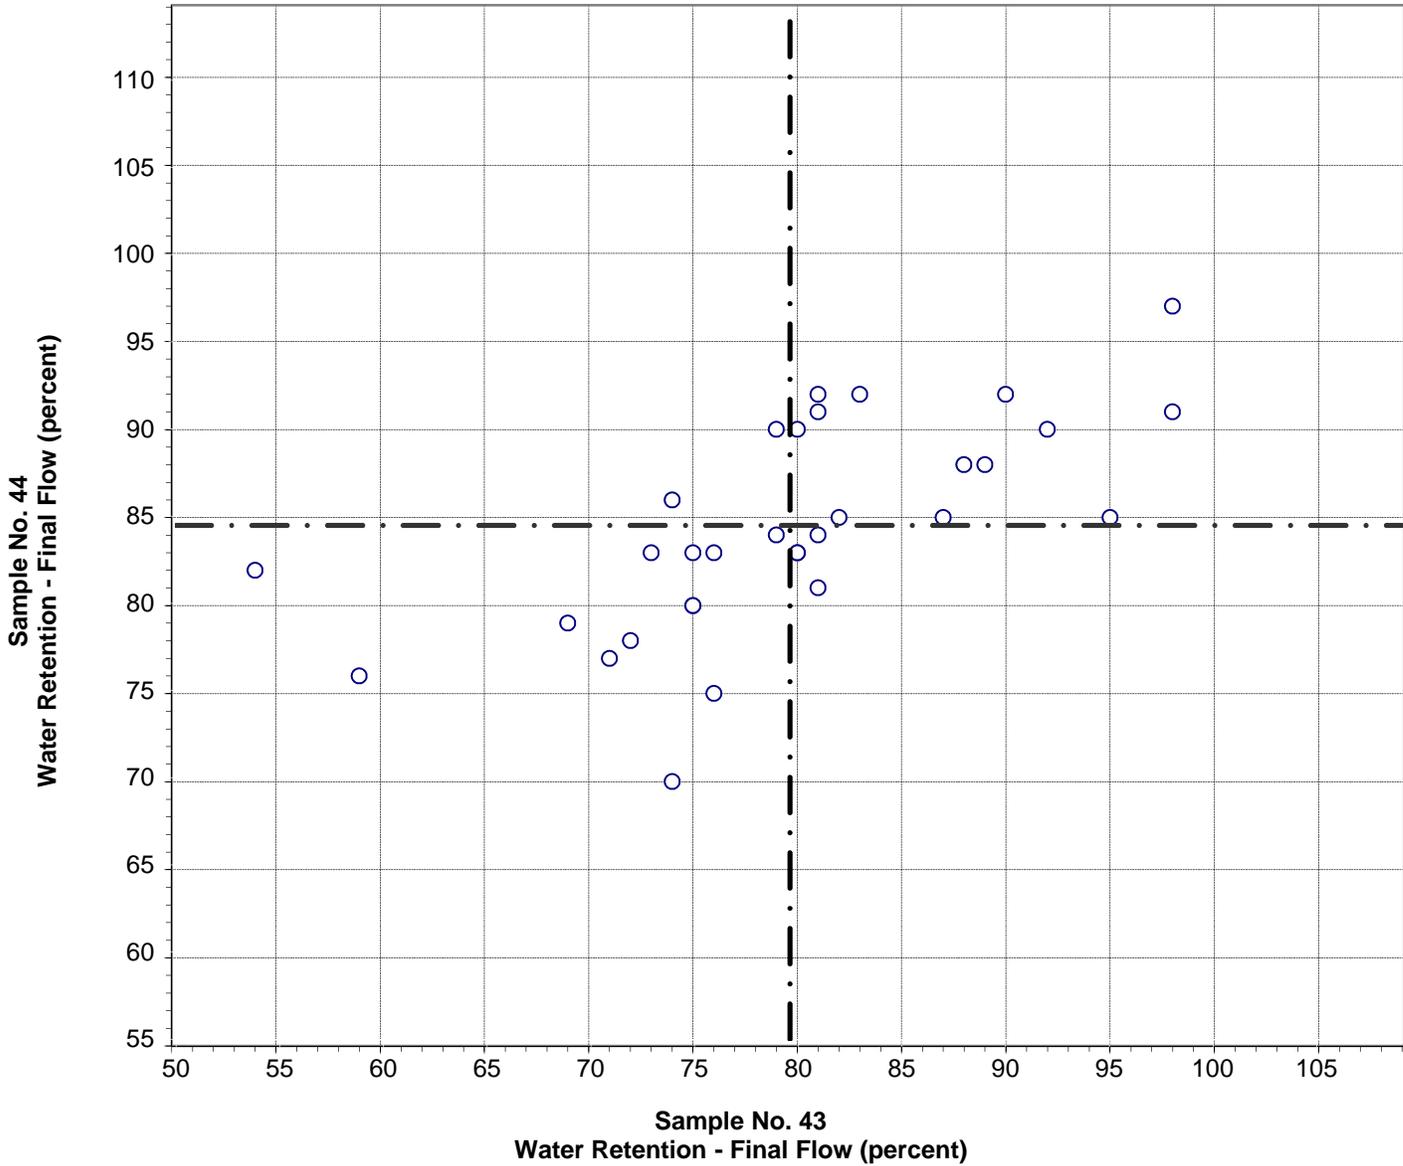

Test No. 332 Water Retention - Final Flow 32 Points

Sample No. 43	Ave 80	S.D. 9.7	C.V. 12.2
Sample No. 44	Ave 84	S.D. 6.0	C.V. 7.1

**CCRL Proficiency Sample Program
Water Retention Value
MASONRY MORTAR Samples No. 43 and No. 44**

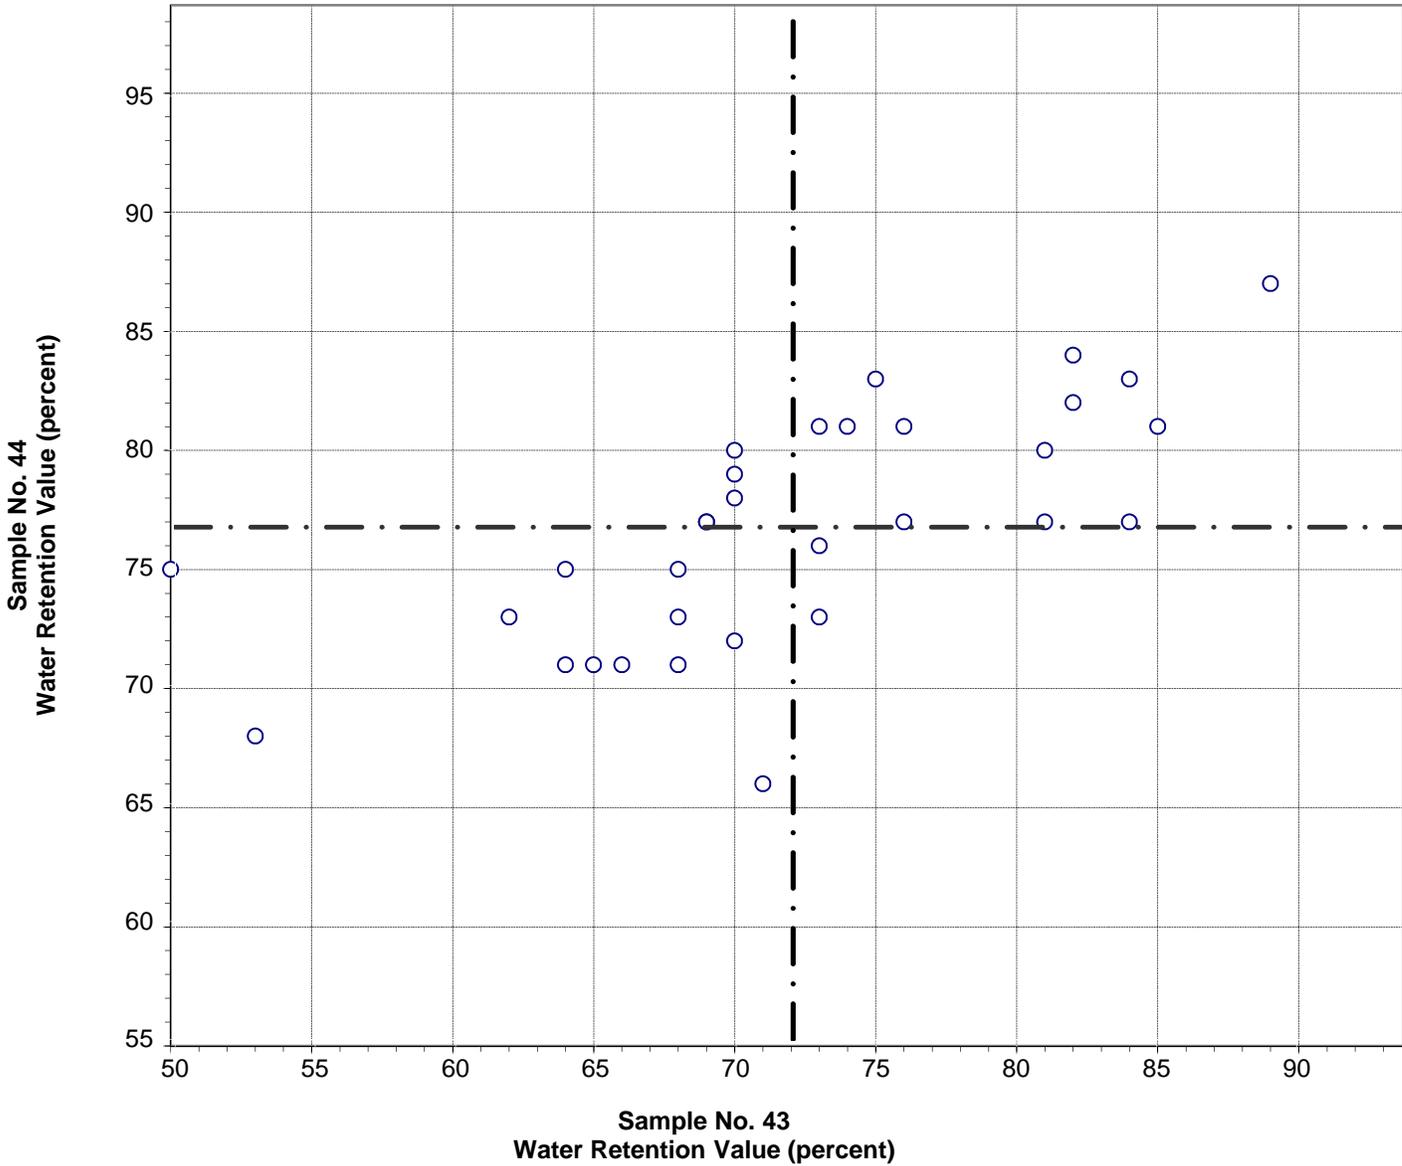

Test No. 333 Water Retention Value 32 Points

Sample No. 43	Ave 72	S.D. 8.8	C.V. 12.2
Sample No. 44	Ave 77	S.D. 5.0	C.V. 6.5